

METHODS AND TECHNIQUES

Development of a deep neural network for automated electromyographic pattern classification

Riad Akhundov^{1,2,3,*}, David J. Saxby^{1,2}, Suzi Edwards⁴, Suzanne Snodgrass³, Phil Clausen⁵ and Laura E. Diamond^{1,2}

ABSTRACT

Determining the signal quality of surface electromyography (sEMG) recordings is time consuming and requires the judgement of trained observers. An automated procedure to evaluate sEMG quality would streamline data processing and reduce time demands. This paper compares the performance of two supervised and three unsupervised artificial neural networks (ANNs) in the evaluation of sEMG quality. Manually classified sEMG recordings from various lower-limb muscles during motor tasks were used to train ($n=28,000$), test performance ($n=12,000$) and evaluate accuracy ($n=47,000$) of the five ANNs in classifying signals into four categories. Unsupervised ANNs demonstrated a 30–40% increase in classification accuracy (>98%) compared with supervised ANNs. AlexNet demonstrated the highest accuracy (99.55%) with negligible false classifications. The results indicate that sEMG quality evaluation can be automated via an ANN without compromising human-like classification accuracy. This classifier will be publicly available and will be a valuable tool for researchers and clinicians using electromyography.

KEY WORDS: EMG, Artificial neural network, Muscle excitation

INTRODUCTION

Surface electromyography (sEMG) is a non-invasive method for recording muscle excitation. Electrodes are placed on the skin surface atop muscle bellies and form a conducting medium through which the electric potential of the underlying depolarizing motor units is measured. The signal measured at the skin surface is produced by a combination of many depolarizing muscle fibres, acquired only after the signal has travelled through various tissues (e.g. connective tissue, fats and skin). Mechanical perturbations of the skin–electrode interface, known as movement artefact, can distort the sEMG (Raez et al., 2006). Furthermore, the signal can be contaminated by electro-technical noise from electronic equipment, ambient noise caused by electromagnetic radiation from power sources (Amrutha and Arul, 2017) and by unequal skin–electrode impedance between bipolar electrodes (Merletti et al., 2001). Handling these sources of noise, while preserving signal integrity for subsequent interpretation, is challenging.

Electromyography (EMG) is widely used in clinical (e.g. characterization of neuromuscular pathologies), biomedical (e.g. modern human machine interfaces) and neurophysiological (e.g. study of human motor control) applications. For example, neuromusculoskeletal models used to study human movement use sEMG to estimate muscle forces and tissue loads inside the human body (Pizzolato et al., 2015). However, neuromusculoskeletal models rely on valid measures of muscle excitation to produce physiologically plausible outputs. Given the inherent potential for signal contamination, sEMG quality must be evaluated prior to use. Signal properties (e.g. signal-to-noise ratio, frequency spectrum, bursts of activation) are commonly evaluated after data acquisition by visual inspection (Raez et al., 2006). However, visual inspection is time demanding and subjective, and requires trained observers. Development of an automated procedure to evaluate sEMG quality both during and following data acquisition would significantly reduce the burden for researchers and clinicians.

A robust solution for automated sEMG evaluation could be achieved using artificial neural networks (ANNs), which are increasingly used for pattern recognition and classification in the field of machine learning (Russakovsky et al., 2015). An ANN is an information-processing system that simulates the function of biological neurons, and consists of multiple interconnected layers and connection weights (Basheer and Hajmeer, 2000). To classify the dataset in the desired manner, the ANN must be trained, during which connection weights and layer variables are adjusted using features extracted from input signals (Subasi et al., 2006). Feature extraction can be performed either by the user, also known as supervised learning, or automatically by the ANN, known as unsupervised learning (Bengio, 2009), with the latter showing increasingly superior performance in recent years (Schmidhuber, 2015). By combining training and prior manual classification, ANNs are subsequently able to choose the best pattern with which to categorize inputs; however, the exact way an ANN learns differs depending on their type, architecture and application. Once an ANN is trained, it can classify new signals by applying the previously learned relationship between input and output.

The paramount performance metric of an ANN is accuracy. In the field of machine learning, accuracy is a technical term referring to the percentage of classifications performed by the ANN that match the true manual classification. Using ANNs, researchers have successfully distinguished between different wrist and thumb movements used to control an active hand prosthesis (Arveti et al., 2007), detected different phases of the gait cycle (Joshi et al., 2013) and differentiated between sEMG acquired from healthy and neuropathic individuals (Sadikoglu et al., 2017), thus demonstrating the potential of ANNs for human movement applications.

In the year 2017, there were 732 publications identified in PubMed using a key word search of ‘surface electromyography’. We anticipate that an automated method to evaluate sEMG quality

¹Gold Coast Orthopaedics Research, Engineering & Education Alliance (GCORE), Menzies Health Institute Queensland, Griffith University, QLD 4222, Australia.

²School of Allied Health Sciences, Griffith University, QLD 4222, Australia. ³School of Health Sciences, University of Newcastle, Callaghan, NSW 2308, Australia.

⁴School of Environment and Life Sciences, University of Newcastle, Ourimbah, NSW 2258, Australia. ⁵School of Engineering, University of Newcastle, Callaghan, NSW 2308, Australia.

*Author for correspondence (riad.akhundov@uon.edu.au)

 R.A., 0000-0001-7770-3677

List of abbreviations

ANFIS	adaptive neuro-fuzzy inference system
ANN	artificial neural network
CNN	convolutional neural network
EMG	electromyography
PNN	pattern recognition neural network
sEMG	surface electromyography

and exclude spurious signals will have widespread practical application. The aims of this study were first to evaluate the performance of five ANNs used to classify sEMG signal quality and, second, to build an automated and robust sEMG classification tool using the best-performing ANN. We hypothesized that ANNs for sEMG classification using unsupervised learning would have superior classification performance in comparison to ANNs using supervised learning, and sEMG evaluation could be automated using an ANN to achieve human-like accuracy (~95%) (Russakovsky et al., 2015).

MATERIALS AND METHODS**Data acquisition**

Three datasets [1: SCOPEX – The University of Melbourne Human Research Ethics Committee (HREC) 11377168; 2: load sharing trials – Department of Defence and Veterans' Affairs HREC 756-14; 3: ARF – Charles Sturt University HREC 2013/185] were combined, resulting in 87,000 individual sEMG signals from various trunk and lower-limb muscles, including rectus abdominis, vastus lateralis, rectus femoris, semitendinosus, biceps femoris, gastrocnemii and gluteus maximus. The five ANNs evaluated were ANFIS, PNN, AlexNet, VGG16 and ResNet50 (described in detail below). Recordings from different trunk and lower-limb muscles, data acquisition systems (1: Noraxon Telemetry 900, 1200 Hz; 2: Noraxon Telemetry 900, 1000 Hz; 3: Trigno Delsys, 1000 Hz) and biomechanics laboratories were included to increase robustness of the ANNs and prevent overfitting to one distinct experimental or laboratory condition.

Signal processing

A standard approach was used for sEMG signal processing. First, a zero-offset correction was performed to remove any direct current value that may be present due to poor grounding. Data were then filtered using a zero-lag second-order Butterworth bandpass filter (30–300 Hz) to remove low-frequency noise caused by movement artefacts and high-frequency noise caused by higher harmonics from the mains, motors or light sources (Lloyd and Besier, 2003; Ruez et al., 2006). The bandpass-filtered signal was full-wave rectified and low-pass filtered with a zero-lag second-order Butterworth low-pass filter ($f_c=6$ Hz) to create a linear envelope (Lloyd and Besier, 2003; White and Winter, 1992).

Manual classification

The sEMG data were manually classified into four categories by one operator as 'good', 'usable', 'noise' and 'no signal' (Fig. 1). Clearly defined signals with a high signal-to-noise ratio were classified as good. Signals where the signal-to-noise ratio was low, but individual bursts of excitation were still distinguishable were classified as usable. Signals where individual bursts of muscle excitation were not distinguishable from noise were classified as noise. Signals with an absence of any noise or bursts of excitation were classified as no signal. To prevent bias towards one category during the ANN training

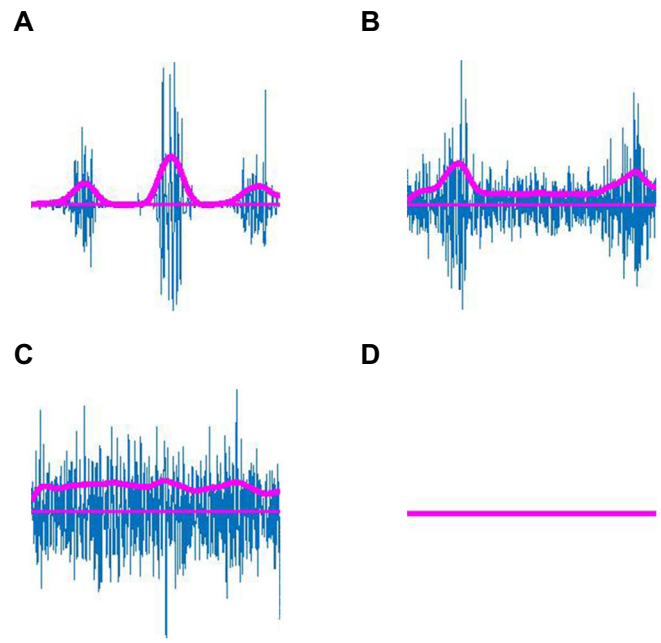


Fig. 1. Visualization of categories for surface electromyography (sEMG) classification. In each plot, the filtered sEMG is displayed (blue), as well as a line at zero (pink; bisecting positive and negative voltages) and the linear envelope (pink; undulating positive signal). (A) 'Good', defined as clearly distinguishable signals with a high signal-to-noise ratio. (B) 'Usable', defined as signals where signal-to-noise ratio was low, but individual bursts of excitation were still distinguishable. (C) 'Noise', defined as signals where individual bursts of excitation were not distinguishable from noise. (D) 'No signal', defined as signals that had an absence of any noise or bursts of excitation.

and in subsequent categorizations, an equal number of samples ($n=10,000$) from all signal categories was used to train all ANNs. This meant that all five ANNs were trained using the same 40,000 of the available 87,000 sEMG signals. These 40,000 samples with equally distributed sEMG quality classifications were then randomized and split into 70% ($n=28,000$) intended for training and 30% ($n=12,000$) for performance evaluation. Separating training from evaluation data is a standard procedure in the field of machine learning, and is designed to prevent erroneously high evaluations of ANN accuracy caused by testing performance on the same data used for training (Dobbin and Simon, 2011). The remaining 47,000 sEMG with uncontrolled classification distribution were used for additional performance testing.

Machine learning

Five ANNs were trained using MATLAB 2017b (MathWorks, Natick, MA, USA). Two were supervised ANNs: (i) adaptive neuro-fuzzy inference system (ANFIS) (Jang, 1993) and (ii) pattern recognition neural network (PNN) (MathWorks). Three were unsupervised ANNs: (i) AlexNet (Krizhevsky et al., 2012), (ii) VGG16 (Simonyan and Zisserman, 2015) and (iii) ResNet50 (He et al., 2016). These five ANNs were selected as they have previously shown promise in delineating motor control tasks via sEMG classification (Arveti et al., 2007; Joshi et al., 2013; Sadikoglu et al., 2017). The ANFIS is a multi-layer feedforward neural network that works on fuzzy logic using 'If-Then' rules as a way of dealing with uncertainty when deciding on the output class of a signal. The combination of fuzzy logic and If-Then rules approximates human information processing and leads to an improved classification accuracy in certain ANN applications

(Güler and Ubeyli, 2005; Jang, 1993). The PNN is a feedforward network-designing tool included in the proprietary programming language MATLAB as part of the Neural Network Toolbox. Here, the number of neurons and the training algorithm can be adjusted to fit the specific dataset, creating a highly customized neural network. AlexNet, VGG16 and ResNet50 are convolutional neural networks (CNNs), i.e. unsupervised neural networks specifically designed for image recognition. An overview of the five architectures can be found in Fig. S1. A CNN classifies images by automatically extracting discriminable features and recognizing patterns therein (Krizhevsky et al., 2012). To be classified by the three CNNs, the sEMG recordings were converted to images (.jpg file format).

ANN training

To train the ANFIS and PNN, a discrete wavelet transform (using Daubechies 7 as the mother wavelet) was first performed on the bandpass-filtered sEMG signals. The following commonly used features were subsequently extracted from the processed sEMG signals (Phinyomark et al., 2012):

$$\text{Mean absolute value} = \frac{1}{N} \sum_{n=1}^N |x_n|, \quad (1)$$

$$\text{Variance of EMG} = \frac{1}{N-1} \sum_{n=1}^N x_n^2, \quad (2)$$

$$\text{Root mean square} = \sqrt{\frac{1}{N} \sum_{n=1}^N x_n^2}, \quad (3)$$

$$\text{Power spectrum ratio} = \frac{P_0}{P} = \frac{\sum_{j=f_0-nl}^{f_0+nl} P_j}{\sum_{j=-\infty}^{\infty} P_j}, \quad (4)$$

where x_n is the n th sample of the sEMG signal, N is the length of the sEMG signal, P_j is the sEMG power spectrum at frequency bin j , f_0 is a feature value of the peak frequency, nl is the integral limit, P_0 is the maximum value of the sEMG power spectrum and P is the whole energy of the sEMG power spectrum in the range 30–300 Hz.

For all three CNNs, the linear envelope was superimposed onto the bandpass-filtered sEMG signal and subsequently converted to an image (Fig. 1). All five ANNs were trained using a combination of manual classification and extracted features or created images, depending on their machine learning category.

Performance assessment

Performance of the ANNs was assessed by four outcome measures: accuracy, false-positives, false-negatives and time demand of classification. Accuracy is the percentage of sEMG signal classifications by the ANN that match a manual classification, and is considered the primary performance outcome metric for this study. False-positives and false-negatives are represented as the percentage of sEMG falsely classified as better or worse quality, respectively. Time demand of classification is the computational time (s) required by the ANN to classify 1000 samples of sEMG on an Intel Core i5-3570 processor with 16 GB of RAM, which are computer specifications a user is likely to have. The computational time demand of classification is important for the practical implementation of the classification tool.

RESULTS AND DISCUSSION

ANFIS and PNN

The computational time demand of classification for the ANFIS and PNN was low (Table 1), but performance of both was unsatisfactory

Table 1. Accuracy, false-positives, false-negatives and time demand for classification using the five artificial neural networks tested

	Supervised learning		Unsupervised learning		
	ANFIS	PNN	AlexNet	VGG16	ResNet50
Accuracy (%)	60.00	70.90	99.55	98.62	99.31
False-positives (%)	30.29	15.89	0.08	0.67	0.06
False-negatives (%)	9.71	13.21	0.38	0.72	0.62
Time demand (s)	0.34	0.29	2.44	28.90	23.47

ANFIS, adaptive neuro-fuzzy inference system; PNN, pattern recognition neural network.

compared with that of the three CNNs. Accuracy was low (60.0%, 70.9%) and both false-positives (30.3%, 15.9%) and false-negatives (9.7%, 13.2%) were high.

CNNs

The CNNs produced better results than either of the supervised learning ANNs (Table 1). Accuracy was >98%, and both false-positives and false-negatives were reduced to <2% in all three CNNs. AlexNet and ResNet50 yielded comparable classification performance, and both were superior to VGG16; thus, they were considered for the automated sEMG classification tool. The performance of AlexNet and ResNet50 is shown in Fig. 2. Generally, the noise and no signal classes had better accuracy than the good and usable classes. False-positives for classification of noise to good amounted to 0.03%. The usable class showed the largest classification uncertainty of the four classification categories (combined false-positives and false-negatives: 1.77–2.73%).

Classification tool

Implementing and testing the two best-performing CNNs on the set of sEMG data not included in ANN training (i.e. the remaining 47,000 manually classified sEMG) confirmed that AlexNet and ResNet50 both had human-like classification accuracy (~95%) (Russakovsky et al., 2015). AlexNet was chosen for use in the automated sEMG classification tool because ResNet50 had a comparatively high computational time demand (23.47 s for ResNet50, 2.44 s for AlexNet).

The sEMG classification tool functions in five steps. First, data stored in c3d file format (commonly used to record synchronized motion and analog data containing sEMG signals acquired in biomechanics laboratories: C3D.org 2018) are imported into the tool and sEMG signals are extracted. Second, sEMG from each c3d file is filtered as described above. Third, images of the processed sEMG recordings are created. Fourth, those images are classified into four categories (i.e. good, usable, noise and no signal). Last, images are sorted into folders based on their category, and classification results are saved in an easily interpretable American Standard Code for Information Interchange (ASCII) file.

Conclusions

The aims of this study were, first, to evaluate the performance of five different ANNs used to automatically classify sEMG quality and, second, to build an automated and robust sEMG classification tool using the best-performing candidate ANN, thereby streamlining data processing, minimizing subjectivity and reducing the burden on researchers and clinicians using sEMG. Unsupervised learning ANNs showed superior classification performance in comparison to supervised learning ANNs, confirming our first hypothesis. The best-performing ANNs, AlexNet and ResNet50, which each demonstrated >99% accuracy, were used to build and test two

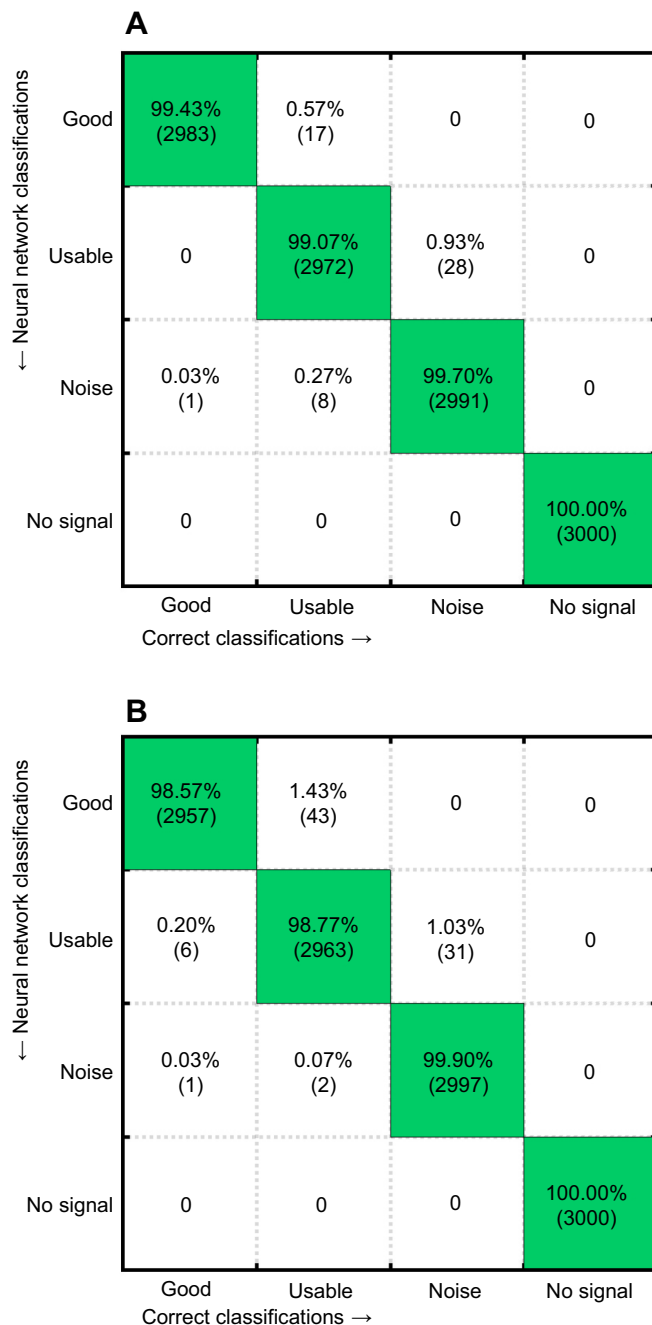


Fig. 2. Confusion matrix for the two convoluted neural networks (CNNs). (A) AlexNet (overall accuracy: 99.55%). (B) ResNet50 (overall accuracy: 99.31%). The horizontal axis shows correct classifications; the vertical axis shows classifications by the neural network; diagonal (green) indicates correct classifications by the neural network. Classification values are presented as a percentage (numerical value).

separate sEMG classification tools. Despite their comparable performance, the computational time demand for ResNet50 was much higher than for AlexNet, and therefore AlexNet was chosen for the final version of the classification tool. The results demonstrate that sEMG classification, which is normally time demanding, tedious and subjective, can be automated using a CNN without compromising human-like classification accuracy. We encourage those interested to contribute manually classified sEMG data to our dataset and to give feedback regarding use of

the sEMG classification tool. Contribution from the scientific and clinical community will help to improve the robustness of this tool.

The results demonstrate that ANNs using unsupervised learning, specifically the CNNs AlexNet and ResNet50, can achieve human-like performance when classifying sEMG quality. This novel observation confirmed our second hypothesis and highlights that labour-intensive, subjective sEMG evaluation can be automated without compromising accuracy. The two ANNs using supervised learning, ANFIS and PNN, showed poor performance metrics due to their respective computational architectures. The ANFIS can handle uncertainty in classification but is unable to account for the high signal variability present in sEMG, which led to a substantial decrease in accuracy. The PNN is specifically designed to fit the sEMG classification task and accounts for this inherent signal variability in the sEMG dataset. This design feature contributed to superior accuracy and fewer false-positives compared with the ANFIS, yet performance of the PNN remained insufficiently robust and did not approach human-like accuracy. The CNNs performed considerably better than both the ANFIS and PNN because the feature extraction and selection from the sEMG signal was performed by the network itself rather than by the user. This aspect of CNNs differs from supervised ANNs, where performance is highly dependent on the appropriateness of selected and extracted features. Hence, a CNN learns directly from the dataset and extracts a high number of relevant features that are empirically determined to be important to the classification of the signal.

Classification accuracy for AlexNet and ResNet50 was similar and excellent. The usable category showed the greatest classification uncertainty with combined false-positives and false-negatives amounting to 1.77–2.73% of the classifications. This observation is unsurprising given that visual inspection of the usable class is challenging and ambiguous for an expert human operator. Computational time demand differences between the two CNNs can be explained by their architectural complexity, i.e. AlexNet consists of eight layers whereas ResNet50 has 50 layers. This time demand means that classifying a set of 1000 images takes ResNet50 approximately 10 times longer than AlexNet, which in turn decreases the practical usefulness of ResNet50 as a within-laboratory or within-clinic tool.

Previous studies using CNNs achieved an accuracy of 99.40% in iris recognition (Minaee and Wang, 2017), 99.95% in palm-print recognition (Minaee et al., 2016) and 90.00% in seizure detection (Acharya et al., 2018). The CNNs in this study showed a performance similar to those of these prior reports, and provide further evidence that robust classification automation can be achieved using unsupervised machine learning. To our knowledge, this is the first study to use CNNs for evaluating sEMG quality and, in combination with the aforementioned studies, highlights that CNNs can be implemented for a variety of clinical applications with excellent outcomes. Limitations of the automated sEMG classification tool presented in this paper should be considered. Because of limited sEMG data availability, the ANNs were trained on datasets from only three different laboratories, and a selection of muscles, experimental tasks and conditions; thus, we cannot guarantee the ANN performance using other datasets acquired in different laboratories or experimental conditions. Although the tool can reliably classify sEMG, its performance for intramuscular or high-density EMG has yet to be evaluated. This study's limitations can be addressed by expanding the training dataset to include samples from different electrode manufacturers, configurations and types applied to different muscles, acquired at different laboratories. To encourage this development, we plan to

make the tool public, with a process for data curation, enabling us to assist other researchers by sharing computational resources.

In conclusion, signal quality from sEMG can be evaluated with >99% accuracy using an automated classification tool. Superior classification performance was achieved by the AlexNet and ResNet50 CNNs compared with the tested ANNs that used supervised learning. AlexNet showed a smaller computational time demand than ResNet50 and consequently was used to build a tool for automated sEMG quality evaluation. This tool demonstrated reliable performance and can be used to streamline data processing without compromising human-like classification accuracy. If implemented during data acquisition, it may also have the potential to quickly identify and thus reduce the number of sEMG recordings with low signal-to-noise ratio. Expansion of the training dataset could further improve the versatility and evaluation performance of the tool.

Competing interests

The authors declare no competing or financial interests.

Author contributions

Conceptualization: D.J.S., S.E., S.S., L.E.D.; Methodology: D.J.S., S.E., S.S., L.E.D.; Software: R.A.; Validation: R.A.; Writing - original draft: R.A.; Writing - review & editing: R.A., D.J.S., S.E., S.S., P.C., L.E.D.; Supervision: D.J.S., S.E., S.S., P.C., L.E.D.; Project administration: S.S., P.C., L.E.D.

Funding

This study was financially supported by the National Basketball Association and General Electric Orthopedics and Sports Medicine Collaboration.

Data availability

To use the EMG classification tool or to contribute your EMG data, please contact the corresponding author (riad.akhundov@uon.edu.au).

Supplementary information

Supplementary information available online at <http://jeb.biologists.org/lookup/doi/10.1242/jeb.198101.supplemental>

References

- Acharya, U. R., Oh, S. L., Hagiwara, Y., Tan, J. H. and Adeli, H.** (2018). Deep convolutional neural network for the automated detection and diagnosis of seizure using EEG signals. *Comput. Biol. Med.* **100**, 270-278.
- Amrutha, N. and Arul, V. H.** (2017). A review on noises in EMG signal and its removal. *Int. J. Sci. Res. Publications* **7**, 23-27.
- Arvetti, M., Gini, G. and Folgheraiter, M.** (2007). Classification of EMG signals through wavelet analysis and neural networks for controlling an active hand prosthesis. 2007 IEEE 10th International Conference on Rehabilitation Robotics, 531-536.
- Basheer, I. A. and Hajmeer, M.** (2000). Artificial neural networks: fundamentals, computing, design, and application. *J. Microbiol. Methods* **43**, 3-31.
- Bengio, Y.** (2009). Learning deep architectures for AI. *Foundations and Trends® in Machine Learning* **2**, 1-127.
- Dobbin, K. K. and Simon, R. M.** (2011). Optimally splitting cases for training and testing high dimensional classifiers. *BMC Med. Genomics* **4**, 31.
- Güler, I. and Übeyli, E. D.** (2005). Adaptive neuro-fuzzy inference system for classification of EEG signals using wavelet coefficients. *J. Neurosci. Methods* **148**, 113-121.
- He, K. M., Zhang, X. Y., Ren, S. Q. and Sun, J.** (2016). Deep Residual Learning for Image Recognition. 2016 IEEE Conference on Computer Vision and Pattern Recognition, 770-778.
- Jang, J. S. R.** (1993). Anfis-adaptive-network-based fuzzy inference system. *IEEE Trans. Syst. Man Cybern.* **23**, 665-685.
- Joshi, C. D., Lahiri, U. and Thakor, N. V.** (2013). Classification of gait phases from lower limb EMG: application to exoskeleton orthosis. 2013 IEEE Point-of-Care Healthcare Technologies, 228-231.
- Krizhevsky, A., Sutskever, I. and Hinton, G.** (2012). ImageNet Classification with Deep Convolutional Neural Networks. NIPS'12 Proceedings of the 25th International Conference on Neural Information Processing Systems 1, 1097-1105.
- Lloyd, D. G. and Besier, T. F.** (2003). An EMG-driven musculoskeletal model to estimate muscle forces and knee joint moments in vivo. *J. Biomech.* **36**, 765-776.
- Merletti, R., Rainoldi, A. and Farina, D.** (2001). Surface electromyography for noninvasive characterization of muscle. *Exerc. Sport Sci. Rev.* **29**, 20-25.
- Miniae, S. and Wang, Y.** (2017). Palmprint Recognition Using Deep Scattering Network. 2017 IEEE International Symposium on Circuits and Systems, 674-677.
- Miniae, S., Abdolrashidi, A. and Wang, Y.** (2016). An Experimental Study of Deep Convolutional Features For Iris Recognition. Proceedings of 2016 IEEE Signal Processing in Medicine and Biology Symposium.
- Phinyomark, A., Nuidod, A., Phukpattaranont, P. and Limsakul, C.** (2012). Feature extraction and reduction of wavelet transform coefficients for EMG pattern classification. *Elektron. Elektrotech.* **122**, 27-32.
- Pizzolato, C., Lloyd, D. G., Sartori, M., Ceseracciu, E., Besier, T. F., Fregly, B. J. and Reggiani, M.** (2015). CEINMS: A toolbox to investigate the influence of different neural control solutions on the prediction of muscle excitation and joint moments during dynamic motor tasks. *J. Biomech.* **48**, 3929-3936.
- Raez, M. B., Hussain, M. S. and Mohd-Yasin, F.** (2006). Techniques of EMG signal analysis: detection, processing, classification and applications. *Biol. Proced. Online* **8**, 11-35.
- Russakovsky, O., Deng, J., Su, H., Krause, J., Satheesh, S., Ma, S., Huang, Z. H., Karpathy, A., Khosla, A., Bernstein, M. et al.** (2015). ImageNet large scale visual recognition challenge. *Int. J. Comput. Vis.* **115**, 211-252.
- Sadikoglu, F., Kavalcioglu, C. and Dagman, B.** (2017). Electromyogram (EMG) signal detection, classification of EMG signals and diagnosis of neuropathy muscle disease. 9th International Conference on Theory and Application of Soft Computing, Computing with Words and Perception, Iccscw 2017 120, 422-429.
- Schmidhuber, J.** (2015). Deep learning in neural networks: an overview. *Neural Netw.* **61**, 85-117.
- Simonyan, K. and Zisserman, A.** (2015). Very Deep Convolutional Networks for Large-Scale Image Recognition. International Conference on Learning Representation.
- Subasi, A., Yilmaz, M. and Riza Ozcalik, H.** (2006). Classification of EMG signals using wavelet neural network. *J. Neurosci. Methods* **156**, 360-367.
- White, S. C. and Winter, D. A.** (1992). Predicting muscle forces in gait from EMG signals and musculotendon kinematics. *J. Electromyogr. Kinesiol.* **2**, 217-231.